




1 / 13

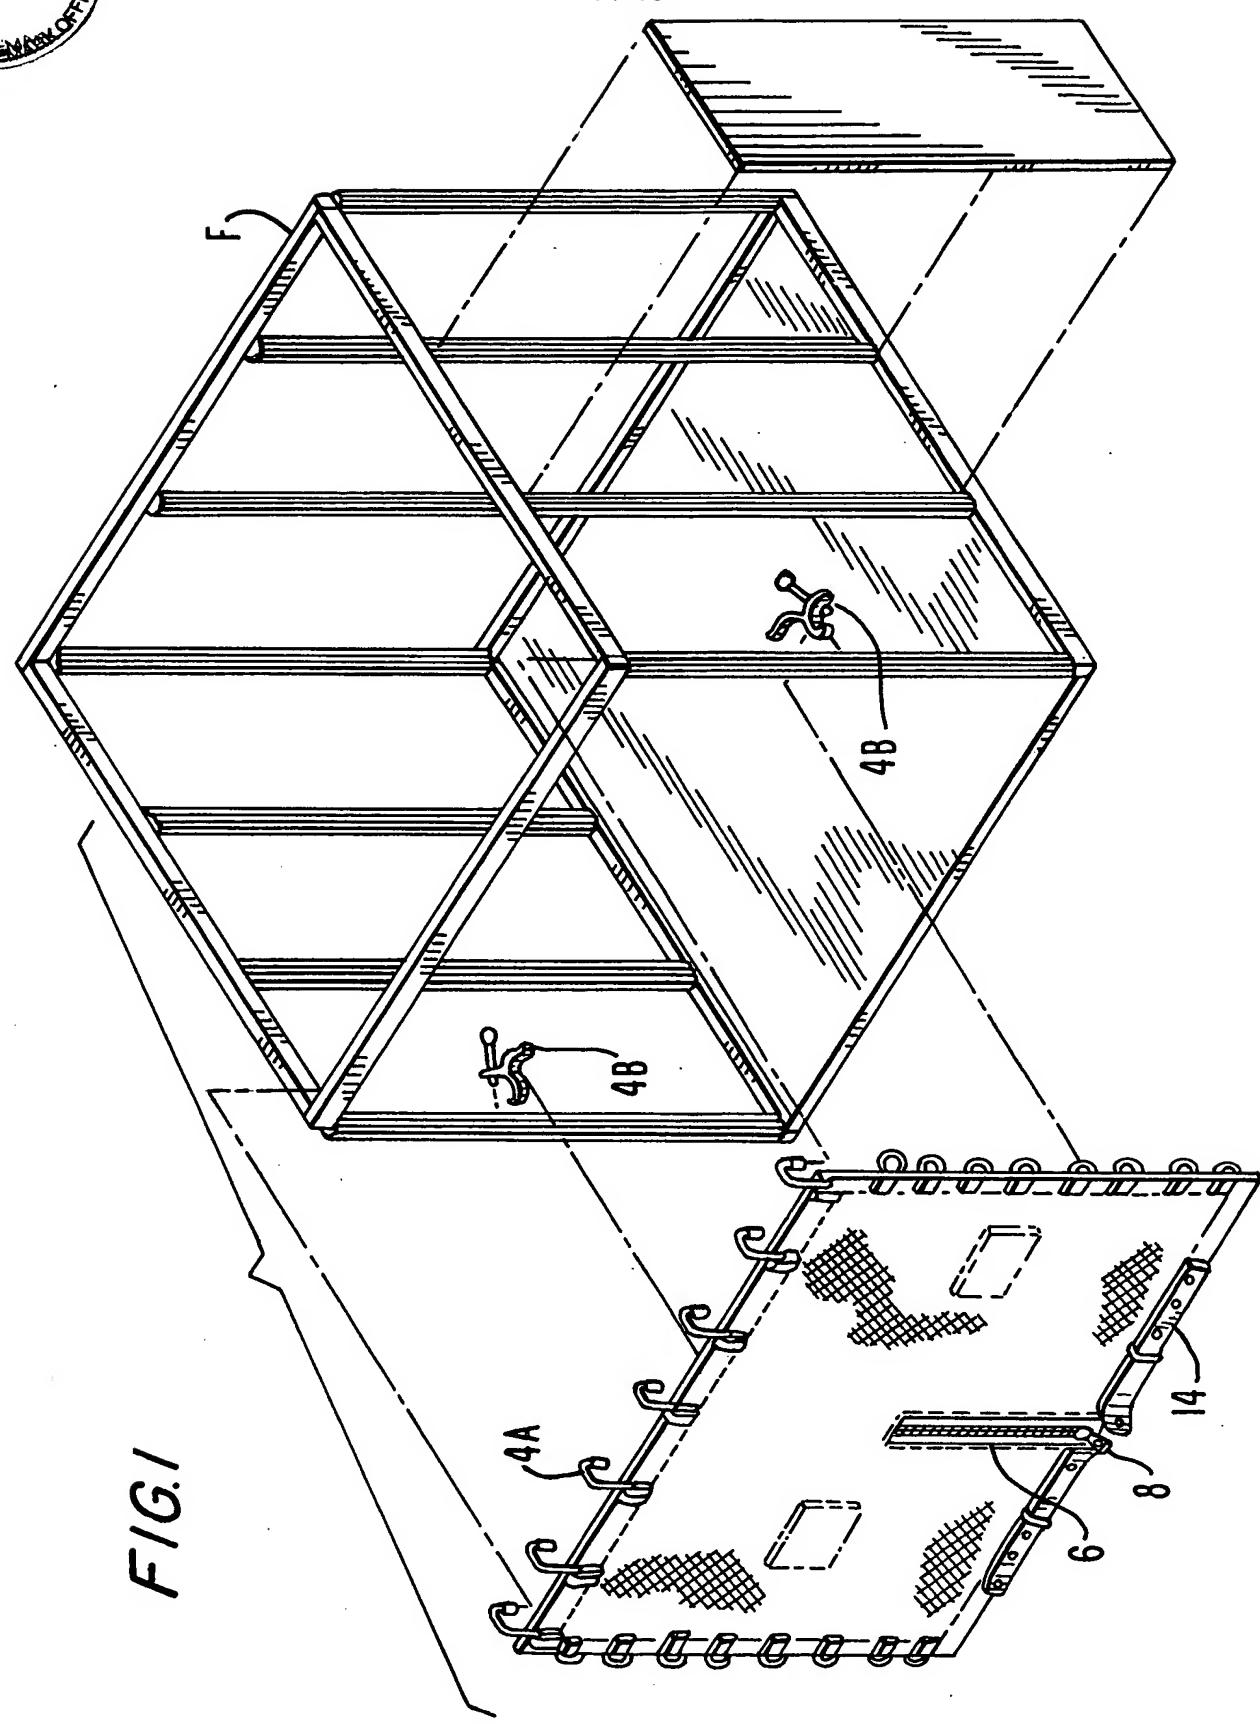

F/G.1

FIG. 2

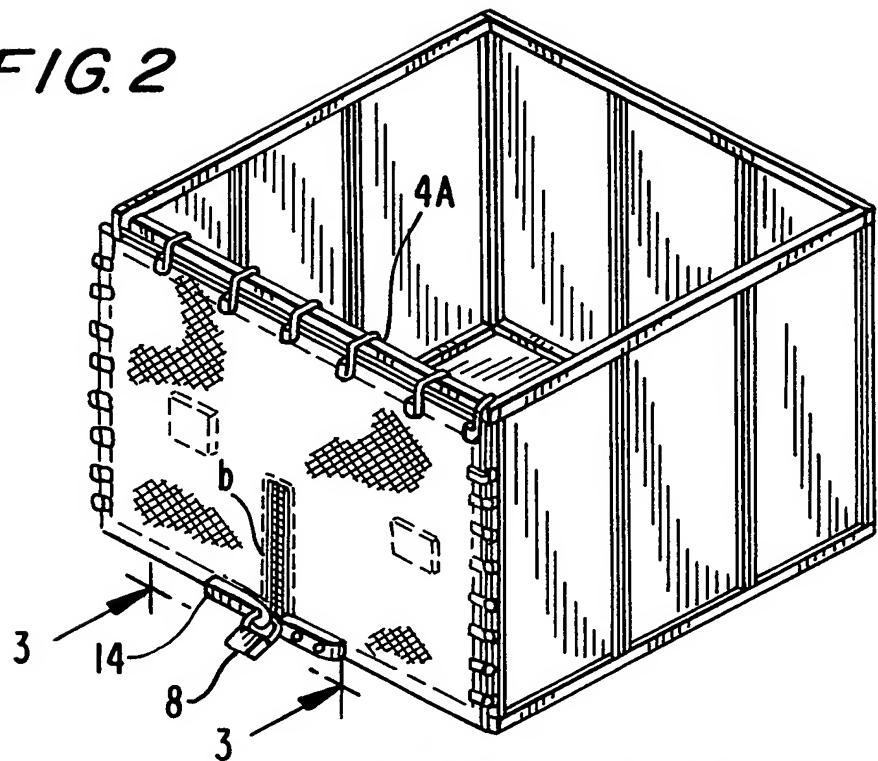


FIG. 3

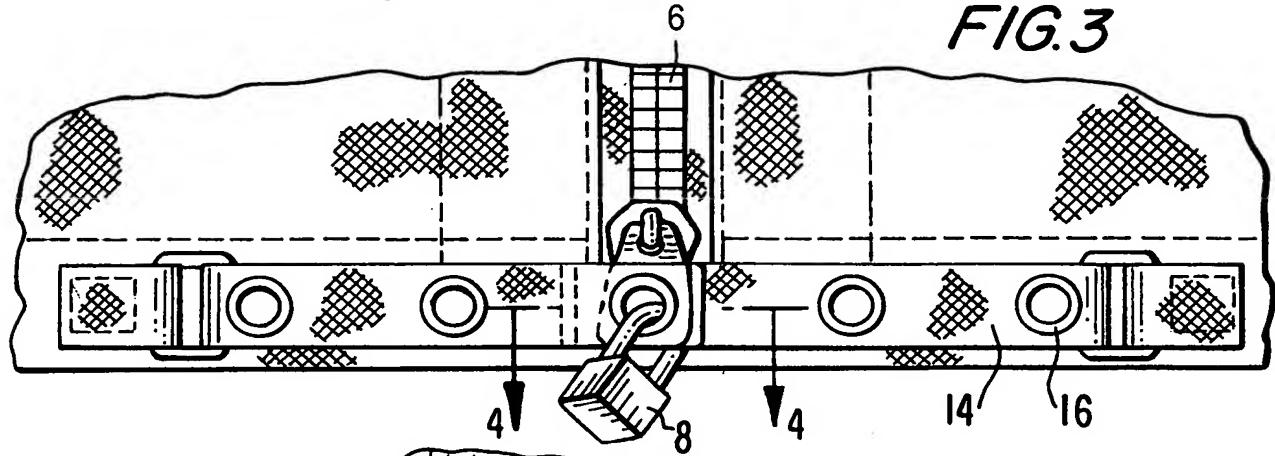


FIG. 4

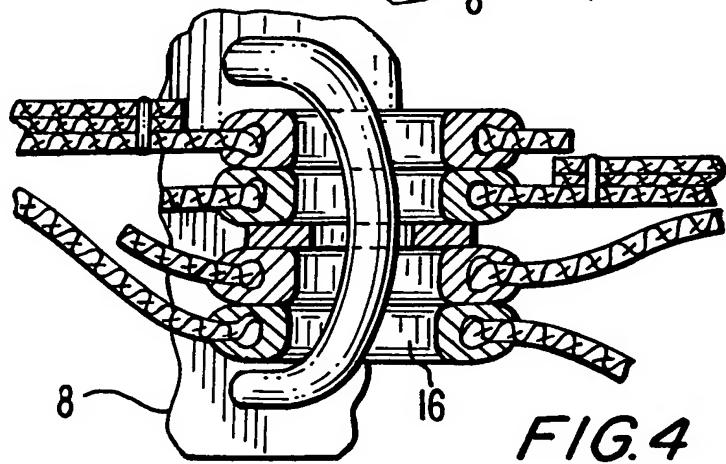
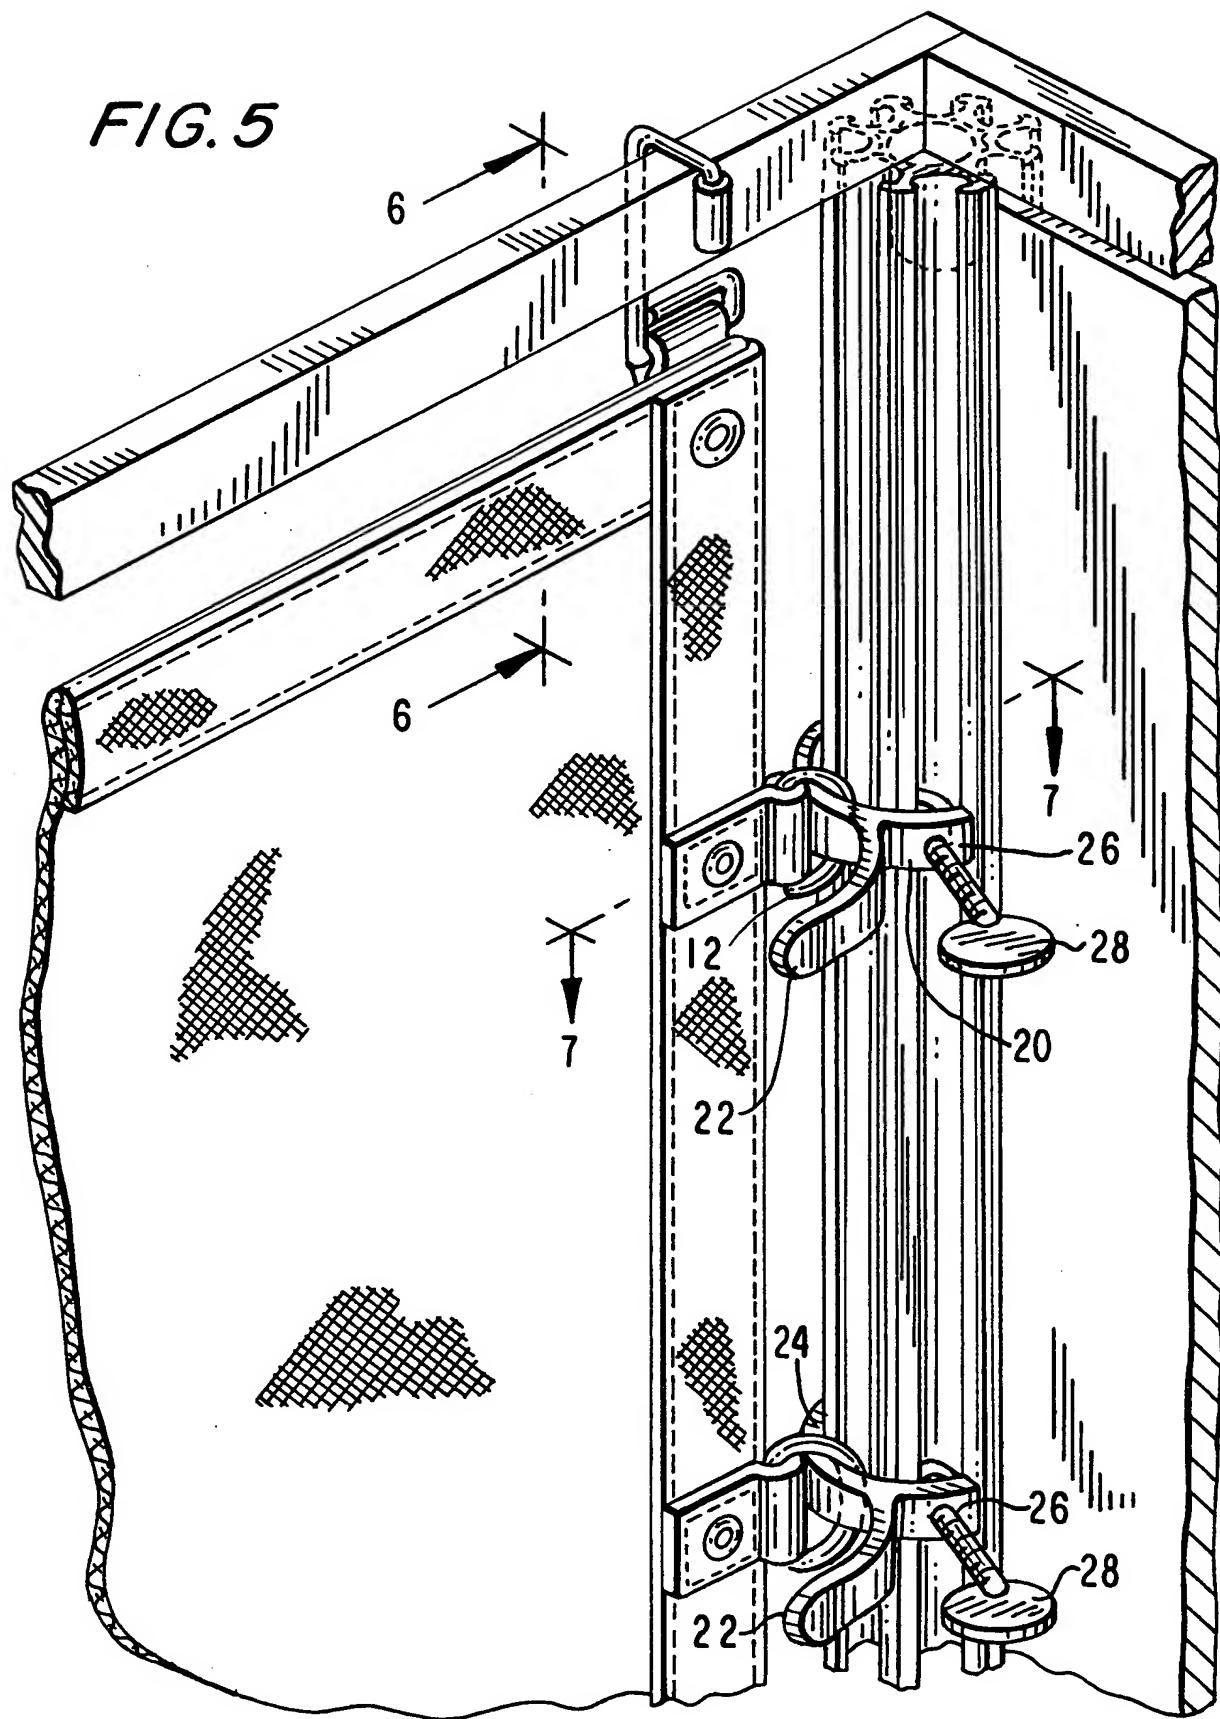


FIG. 5



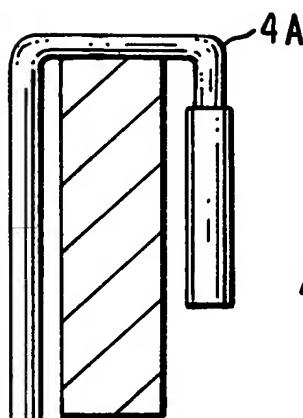


FIG. 6

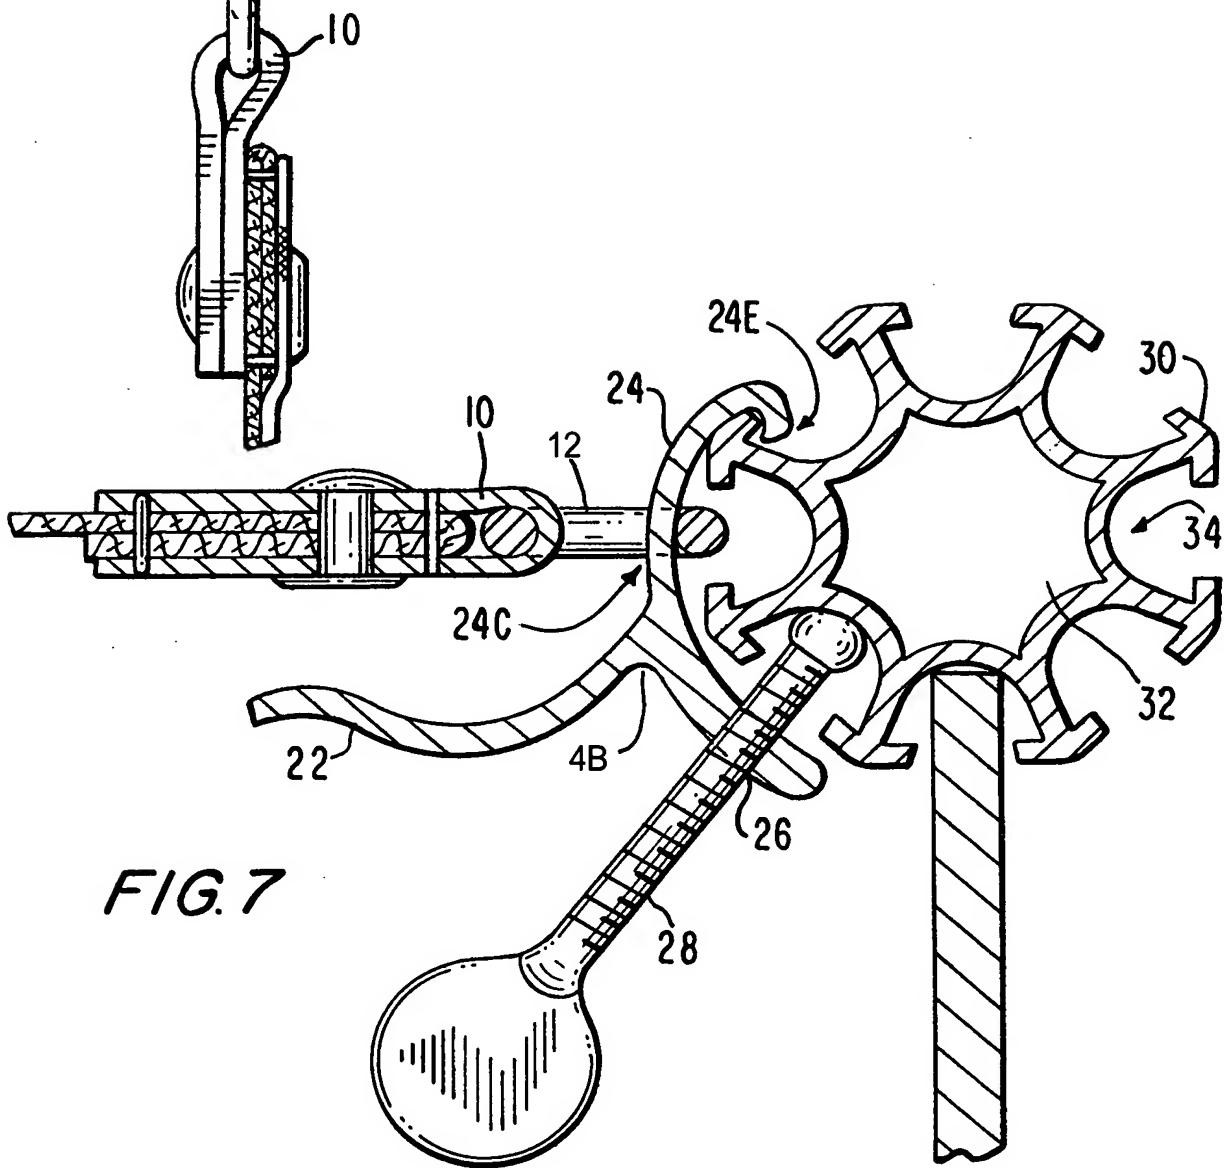


FIG. 7

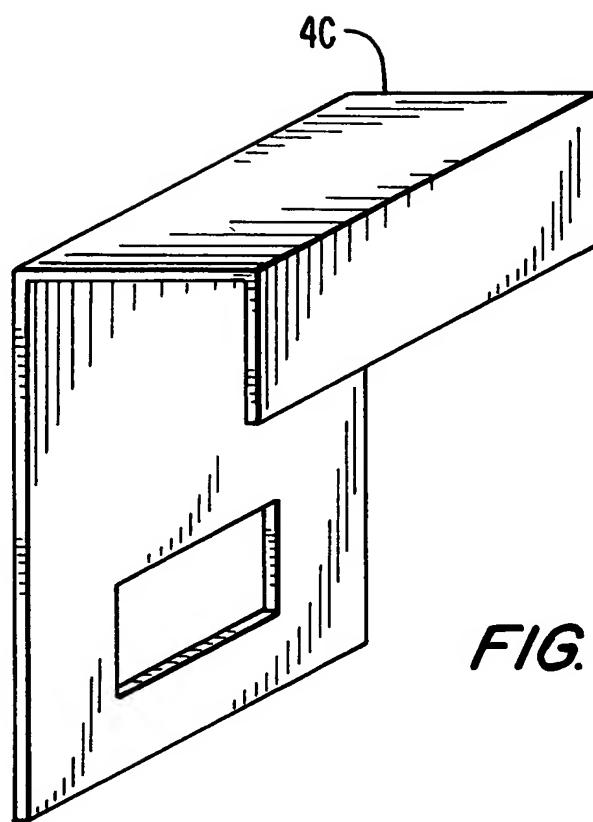
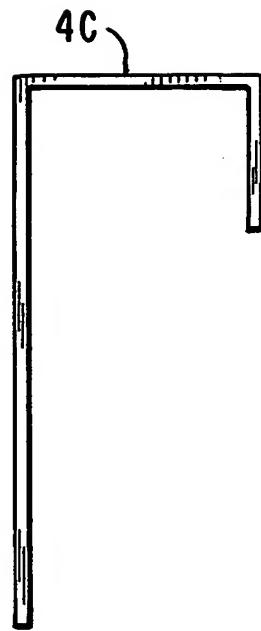
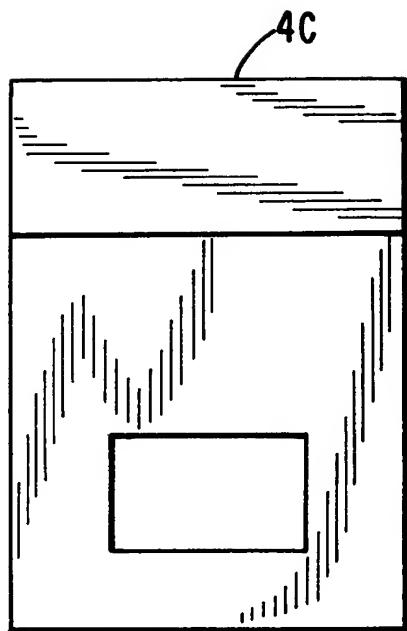


FIG. II

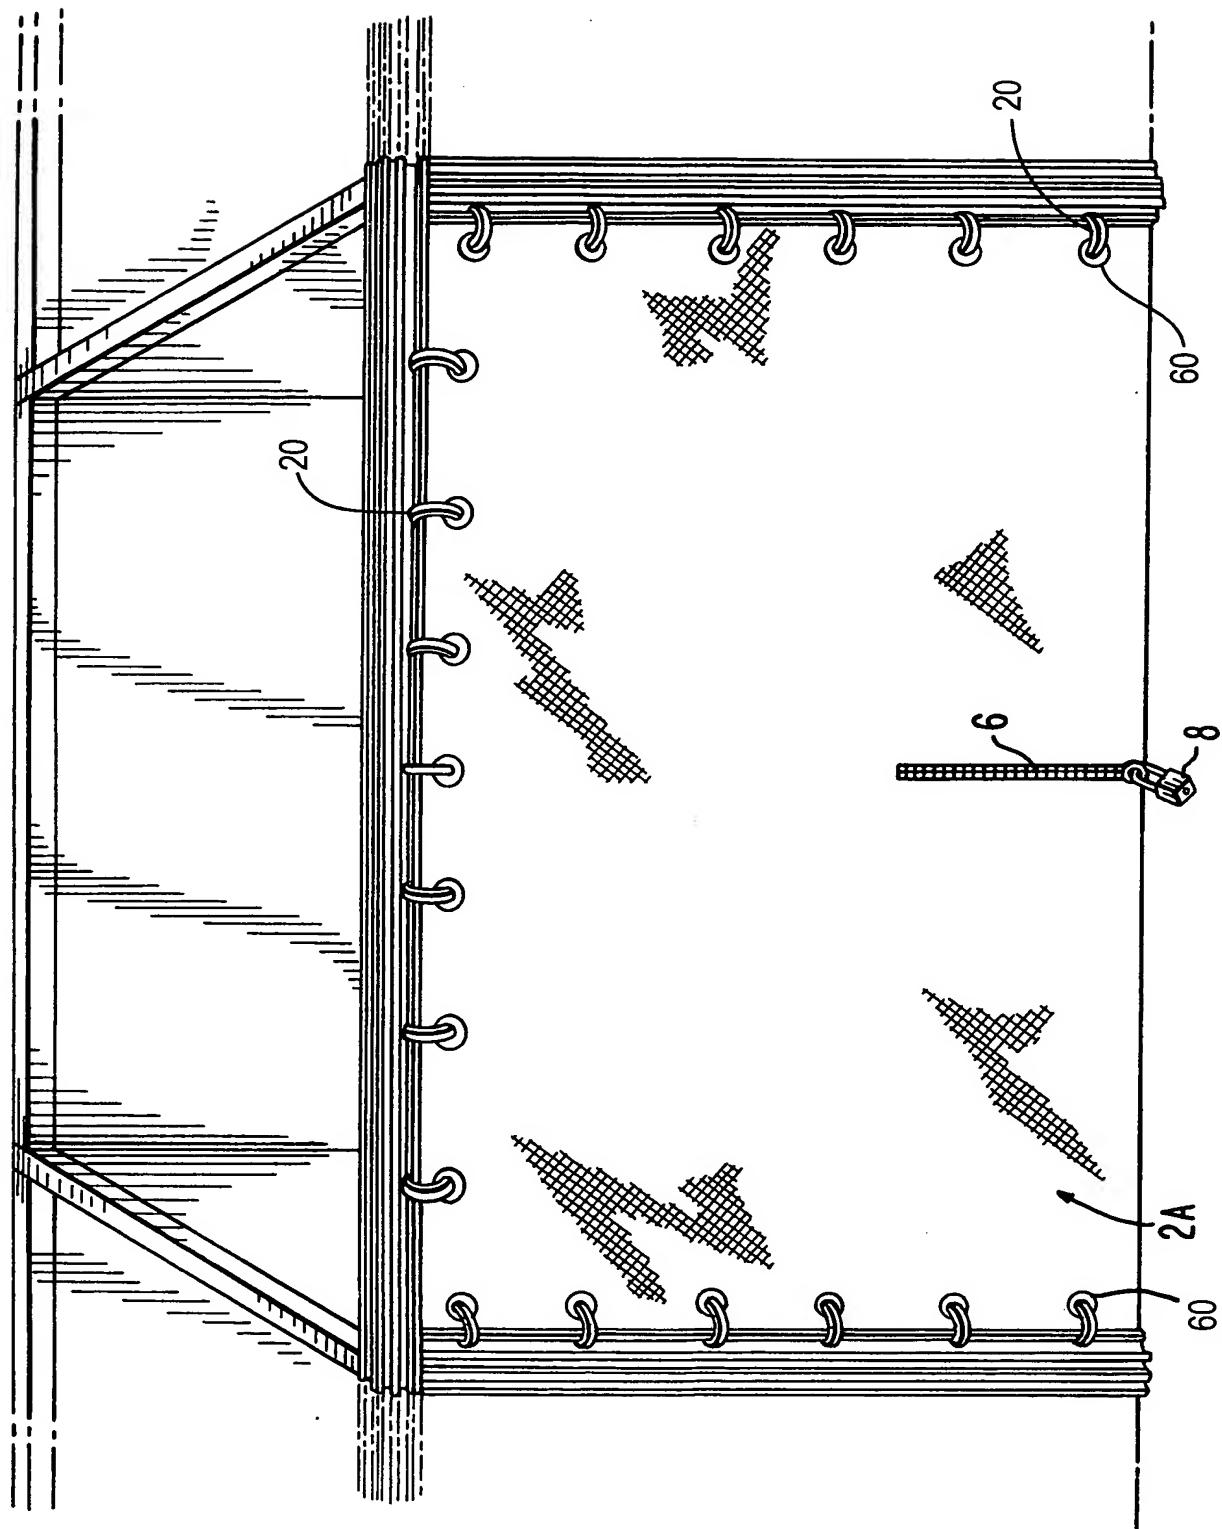
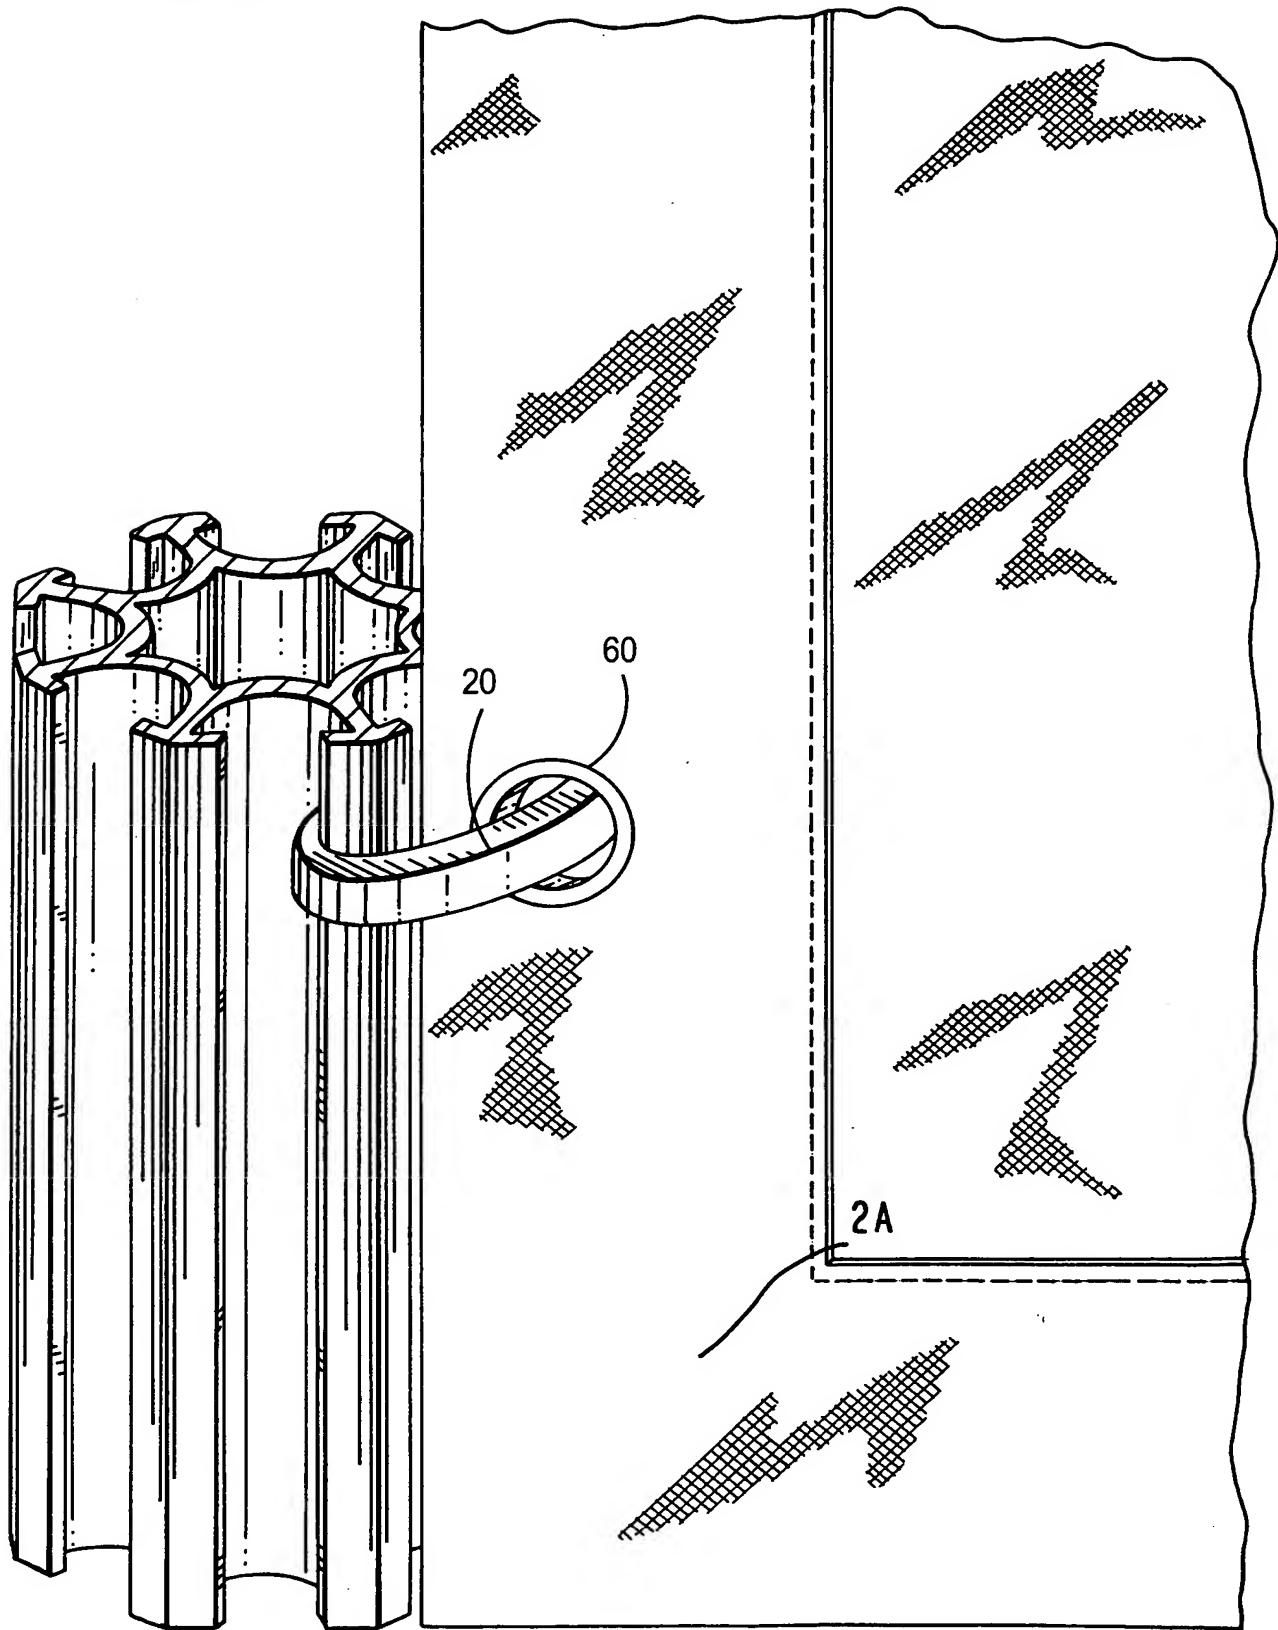


FIG. 12



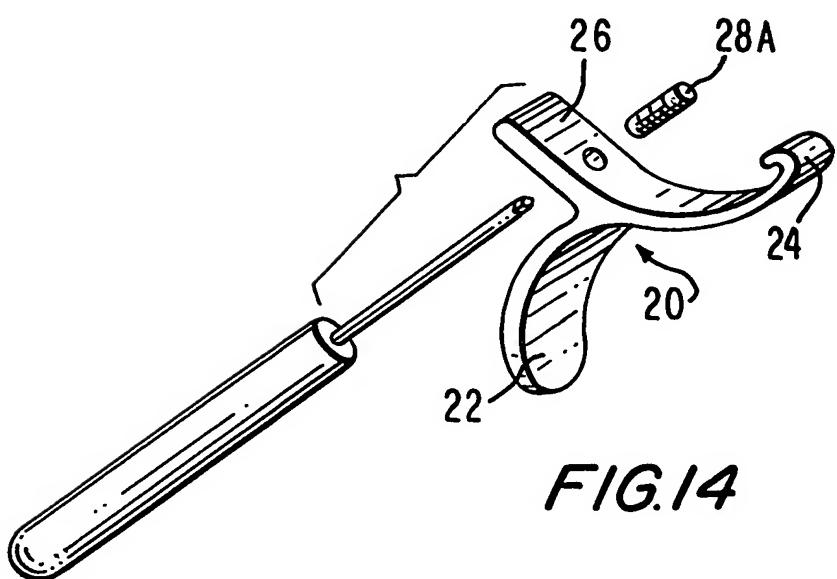
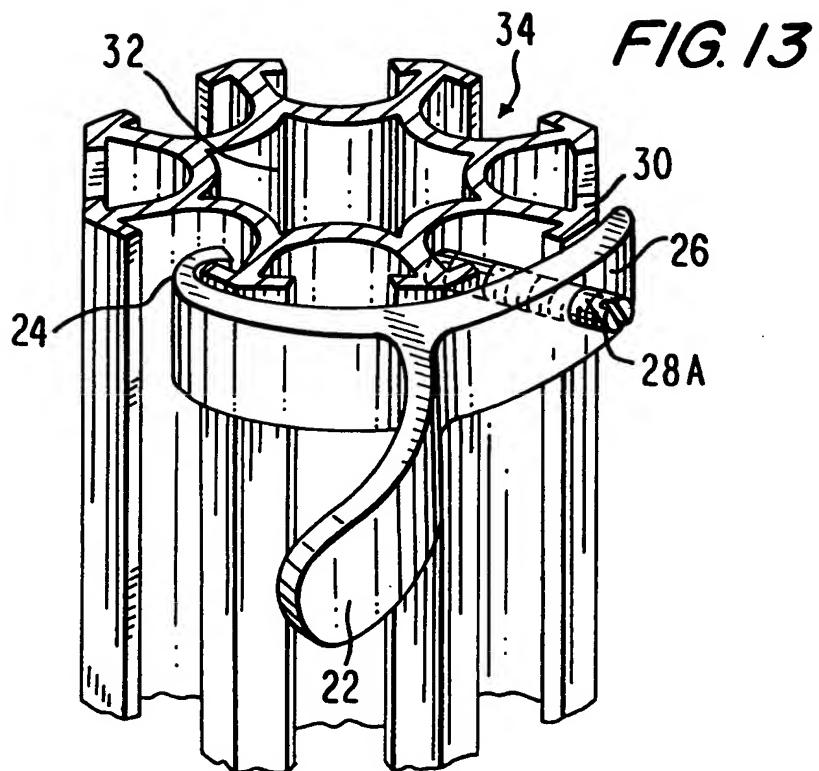
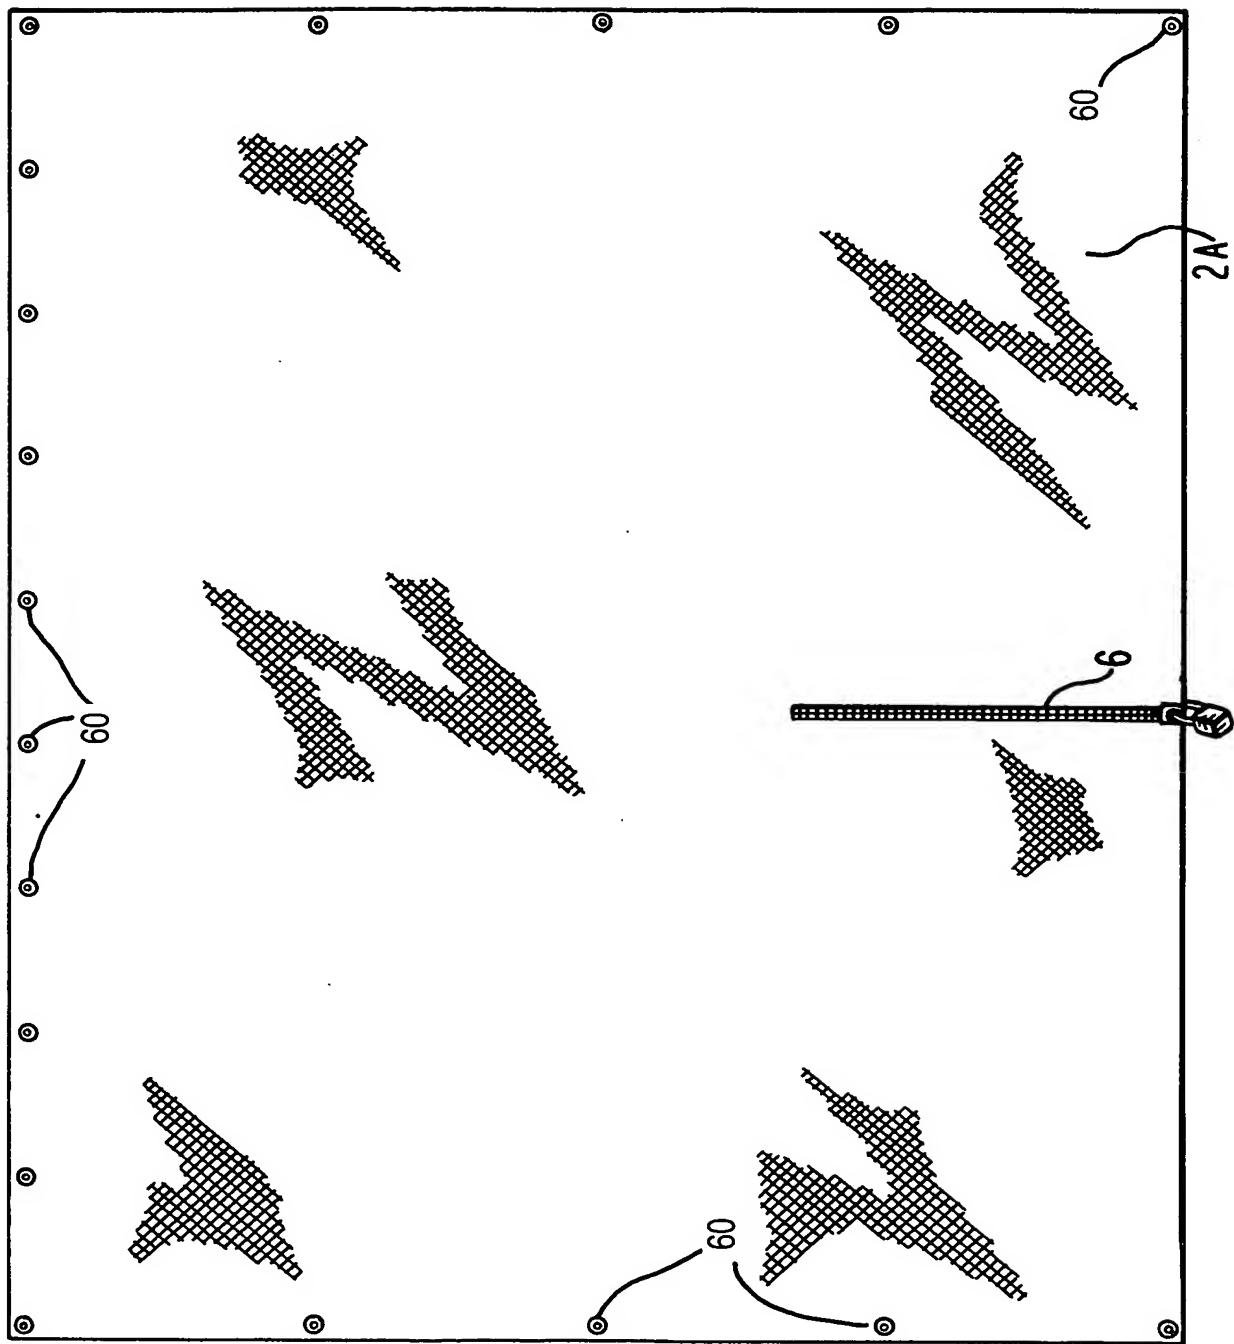


FIG. 15



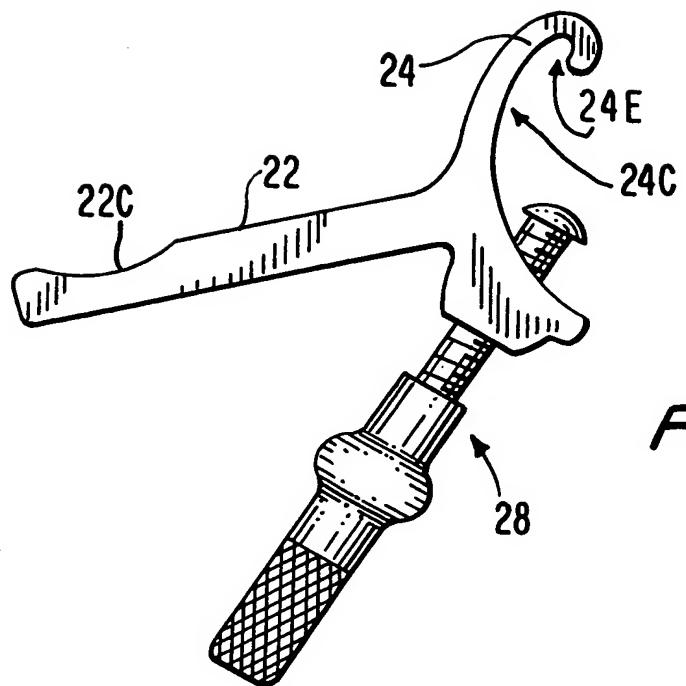
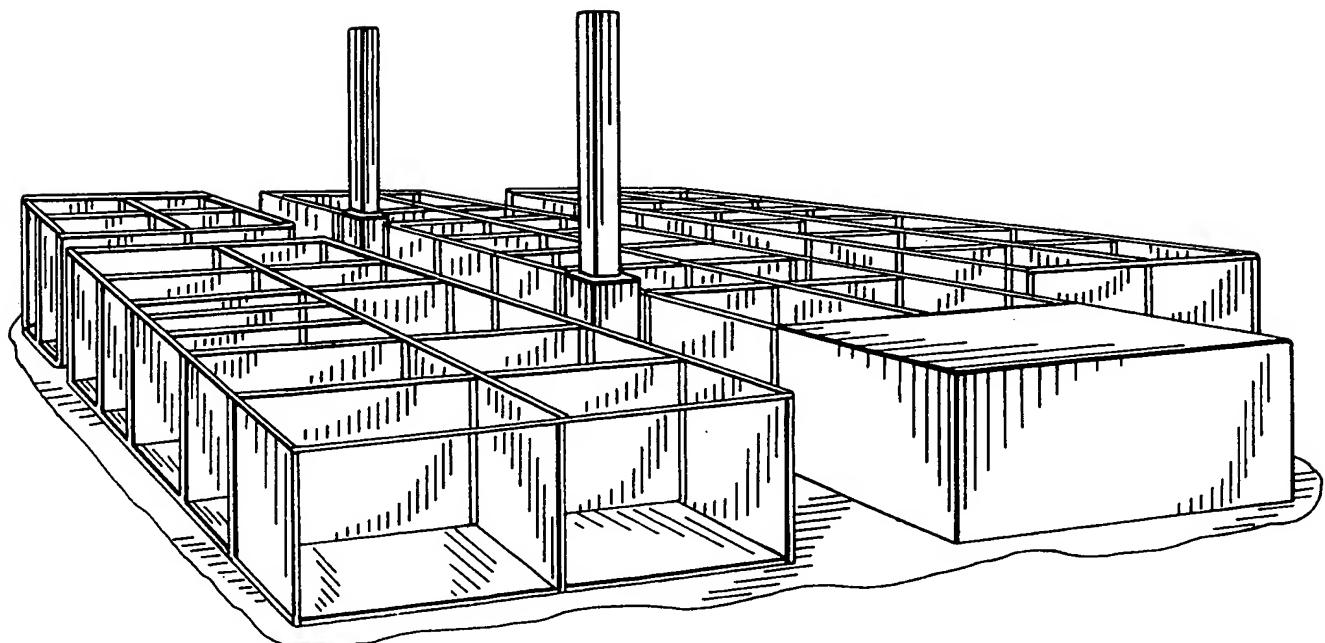
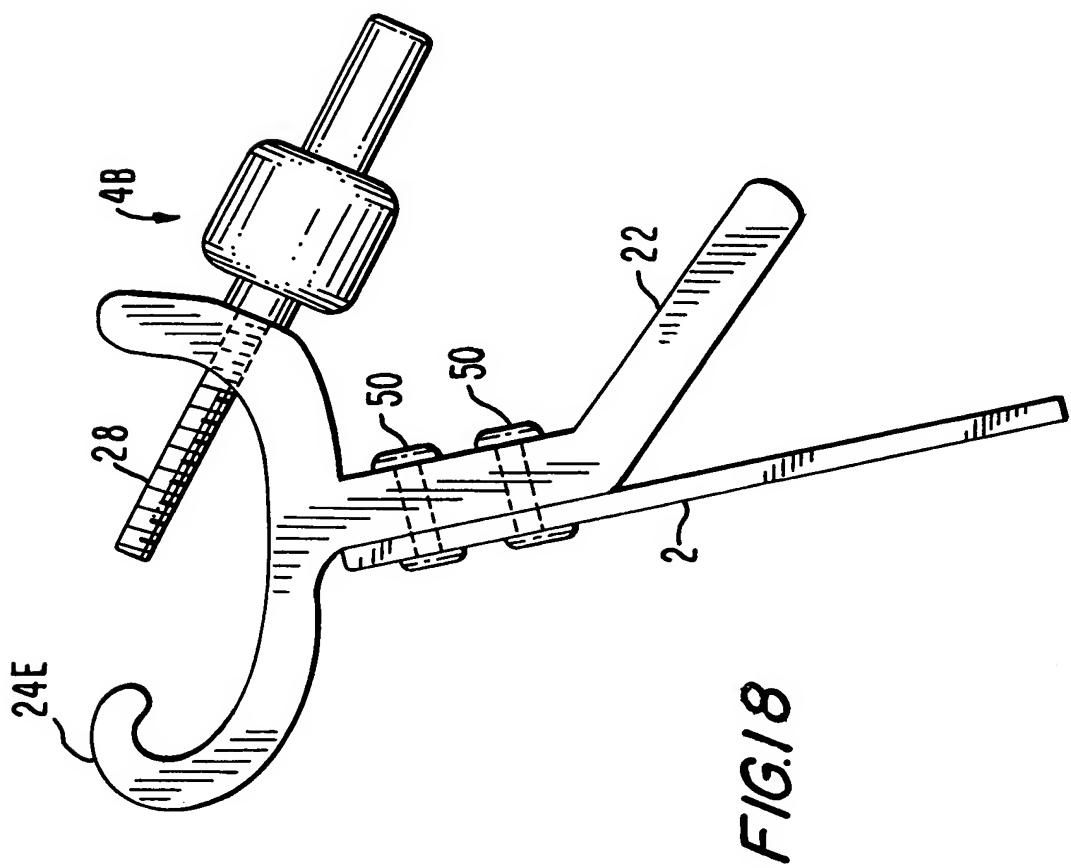
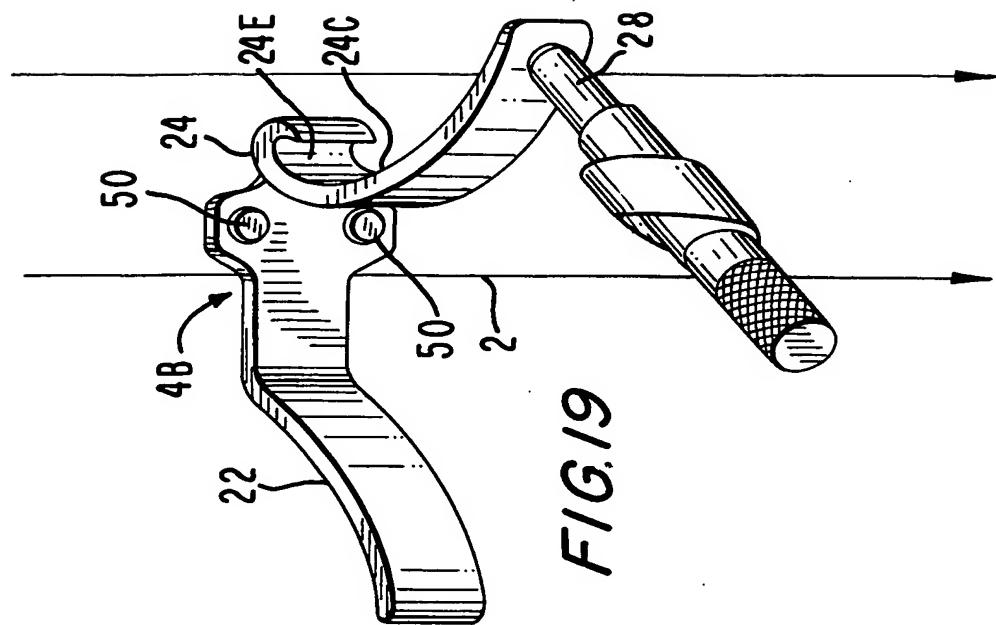
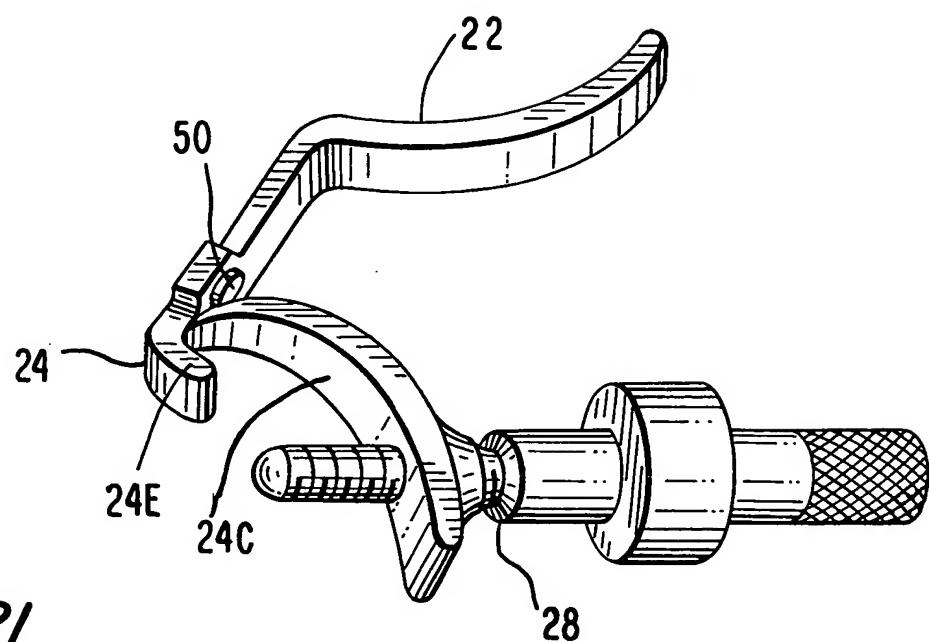
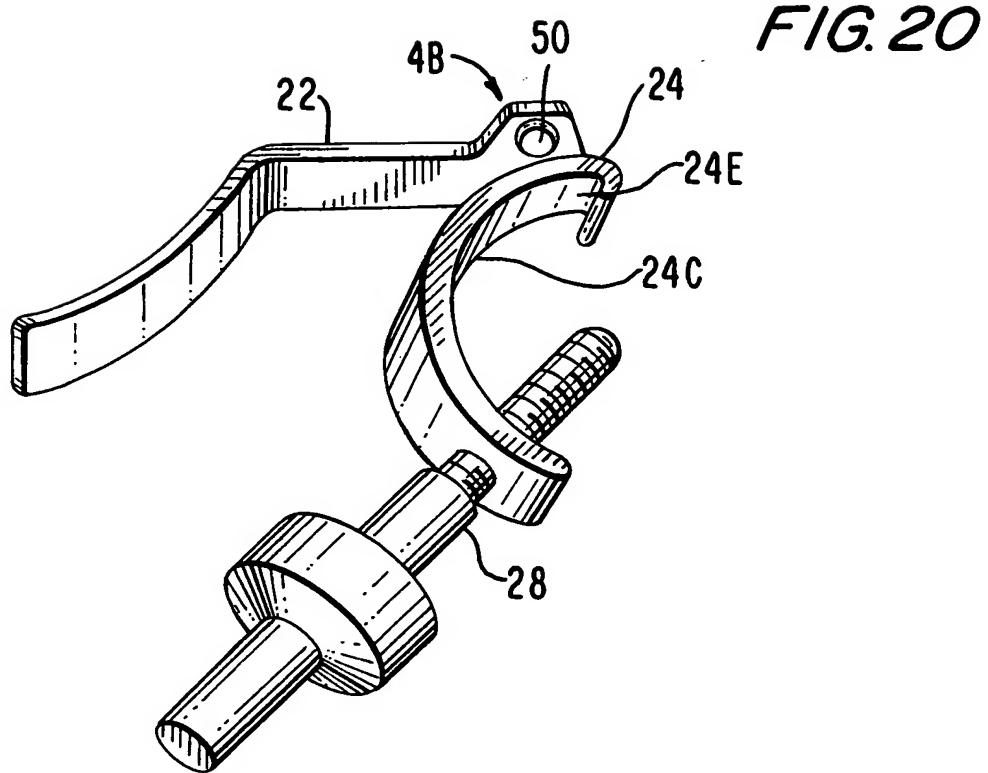


FIG. 17







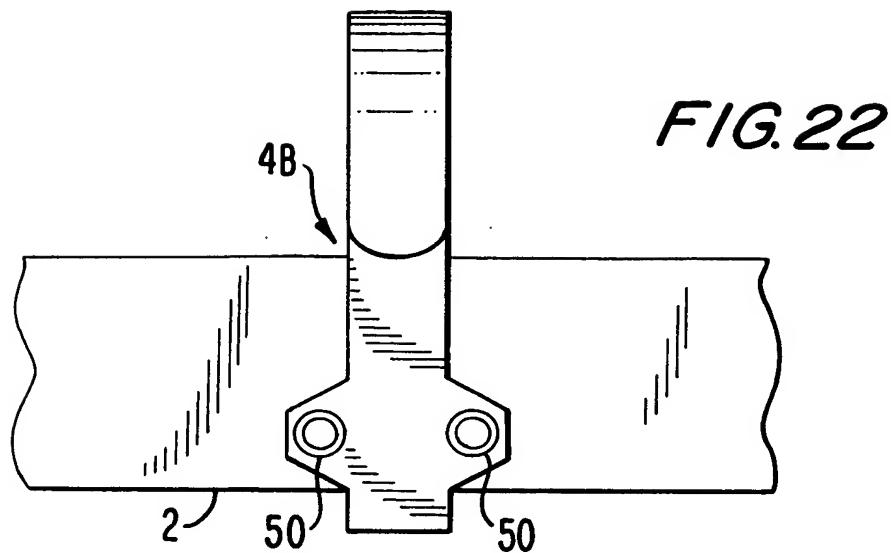


FIG. 22

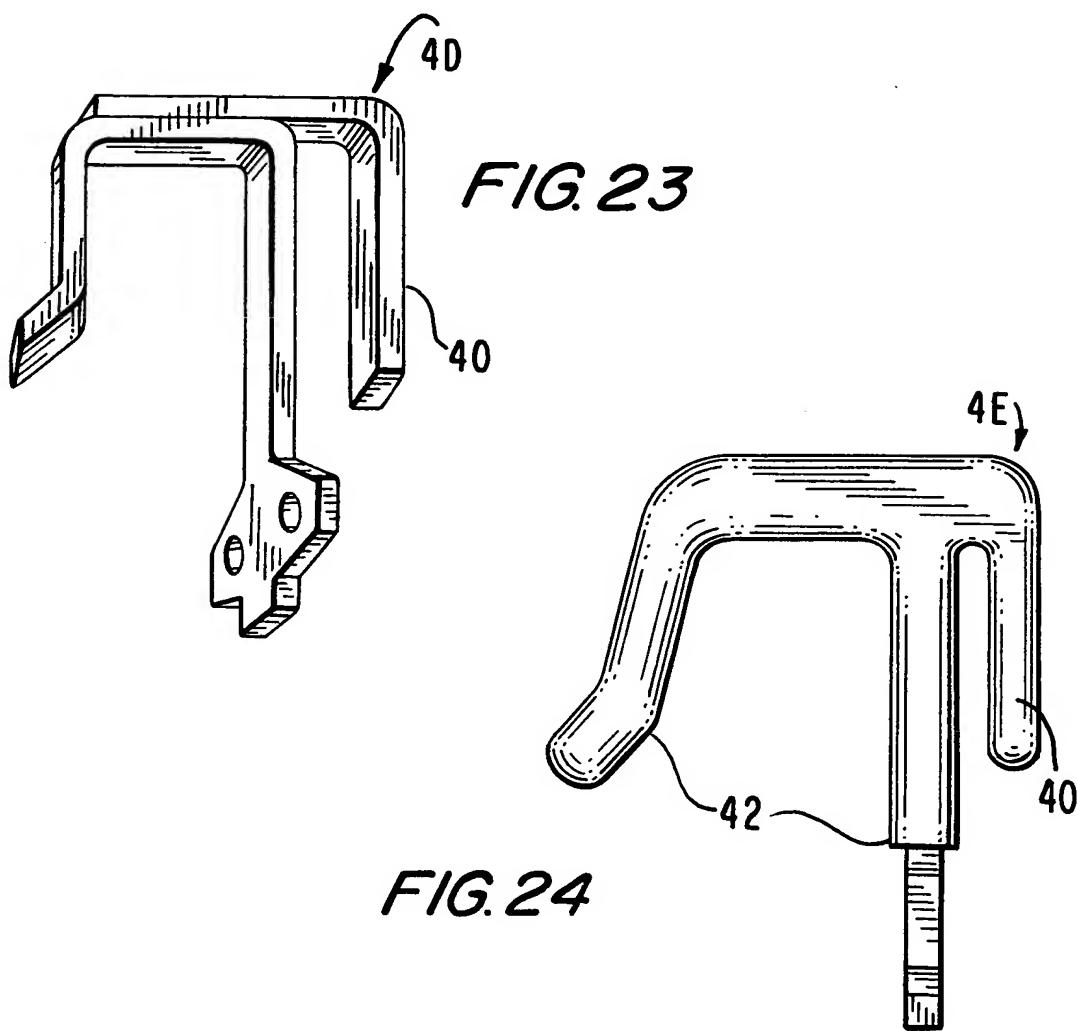


FIG. 24